

AI Binocular Thermal Imaging System Quick Instruction Manual



Version: V1.0

Contents


1. Product Introduction	3
1.1 Product Description	3
1.2 Product Appearance	3
2. Device Installation	4
2.1 Installation Position	4
2.2 Installation Environment Standard	4
3. Quick Instructions	4
3.1 Device Connection	4
3.2 AI Thermal Imaging Screening System	5
3.2.1 Main Interface Introduction	5
3.2.2 Snapshot Folder	6
3.2.3 Setting	6
4. Device Upgrade	7
4.1 Web Upgrade	7
4.2 Tool Upgrade Program:	8

1. Product Introduction

1.1 Product Description

This Intelligent AI binocular thermal imaging system is composed of AI binocular temperature detecting camera and AI thermal imaging screening system. Integrated by thermal temperature detecting sensor of high-accuracy, built-in intelligent face capture algorithm, and ISP image processing technology etc, this device is with face detection, temperature detection and face capture, etc powerful features. With AI thermal imaging screening system, it can accurately detecting the body temperature, capturing face pics and records for those people appeared in front of this device. It can effectively help to monitor and detect the body temperature of entry and exit people, thus contributing to prevent epidemic situation. It can be widely used at all kinds of entrances and exits of school, buildings, stations, etc.

1.2 Product Appearance

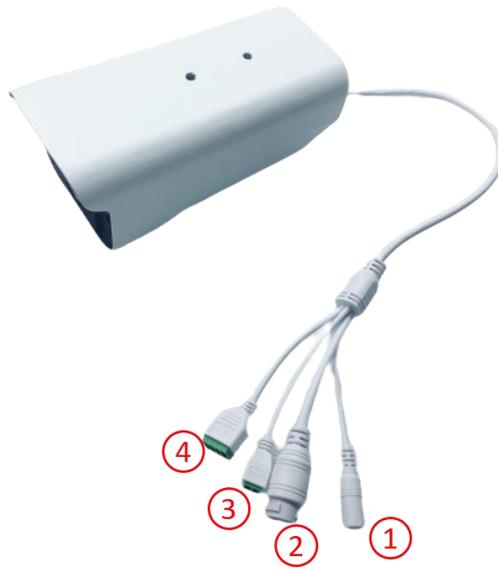

1.3 Device Interface Function Definition

Interface No.	Interface Name	Functional Indicators
1	Power Interface	12VDC
2	Network Interface	RJ45 Network Interface
3	Relay Interface	+ : NO Normally Open Port - : COM Public Port
4	Audio Interface	1: Audio Input 2: Audio Ground 3: Audio Output 4: Empty


2. Device Installation

2.1 Installation Position

1. Camera being set in front of the aisle to capture the face;
2. Suggested installation height is about 2 meters, and camera over look view angle $0^{\circ}\sim 15^{\circ}$;
3. For accurate detection of body temperature, 1 meter (Range 1m to 2.5m) distance is tested for the optimum capture distance.

2.2 Installation Environment Standard

1. Illumination Requirements: No back light, no obviously reflect light on face, uniform light and no shadow. In addition, to ensure the enough illumination of the scene when capturing the face, it is suggested to increase the lighting devices if the face in the display is not bright enough which may affect the face capture (General 250~800Lux).
2. Light and Wind Requirements: This Device is suggested to be installed indoor, ensuring there is no wind between device and people, no direct sunlight, so as to avoid the detected temperature too low or too high caused by blowing, cooling and direct sunlight.

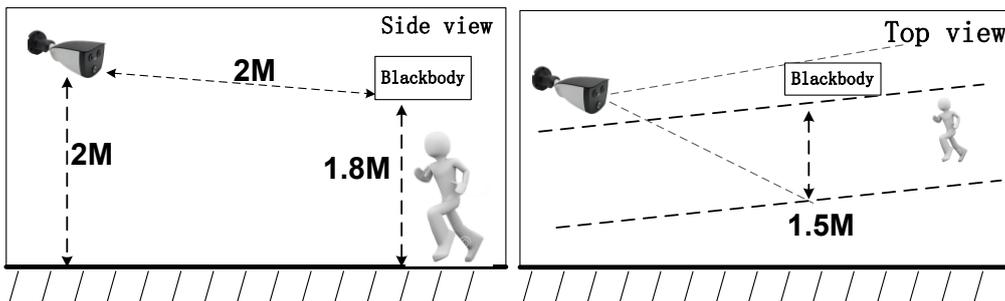


3. Quick Instructions

3.1 Device Connection

Connect the device to the computer correctly through network cable; after the device powered on, open the search tool on the computer, search device IP address. User can also modify the IP address by search tool at the same time.


Notice: Default device IP address is 192.168.1.18.

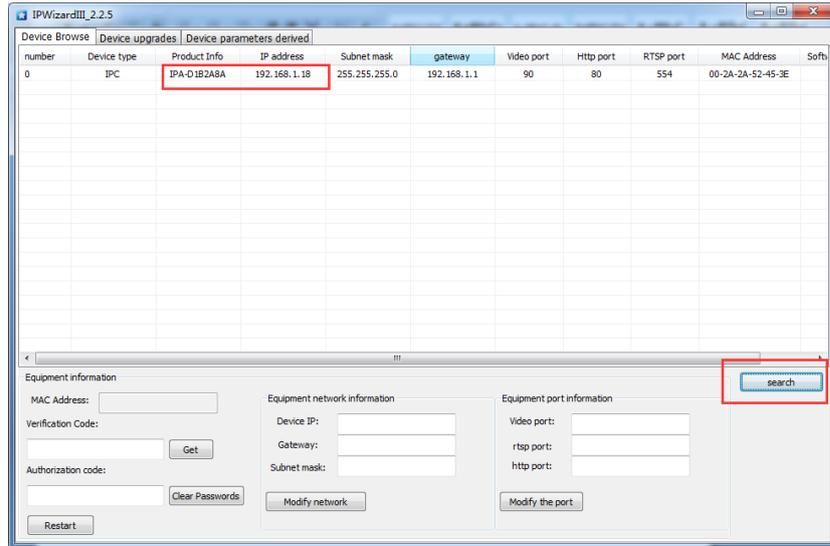

3.2 AI Thermal Imaging Screening System

After device powered on, user can use AI thermal imaging screening system software to connect device, preview, setting, alarm clean, snapshot pic preview, export records, etc operation.

3.2.1 Main Interface Introduction

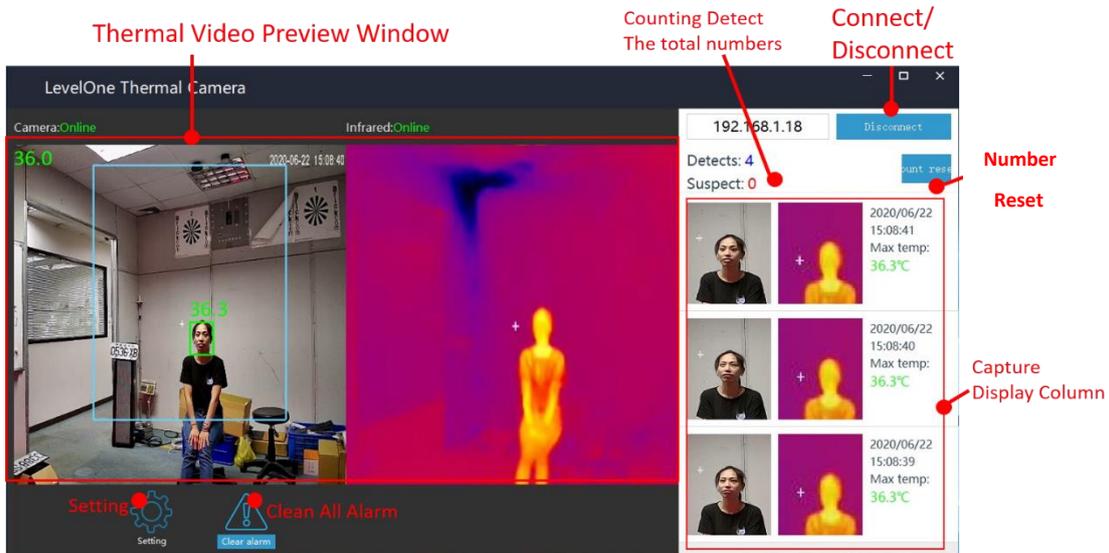

【Video Preview Window】 : After device connected, user can view double screen(optical and thermal imaging)for real-time preview as above pic shows;

【IP Input Box】 : Input device’s IP address. The device default IP address is 192.168.1.18;

【Connect/Disconnect Device Button】 : Click **【Connect】** to view the real-time display, face capture pic and temperature detecting. Click **【Disconnect】** to close the preview;

【Capture Display Column】 : List the current captured face pic and detecting temperature;

【Snapshot Folder】 : Click the snapshot folder to check saved captured face;

【Setting】 : Click to modify the settings for face capture and temperature detecting alarm;

【Clear Alarm】 : After click, the alarm will be canceled;

【Detects】 : Counting the total numbers of face capture and shows;

【Suspect】 : Counting the total number of face capture for those above the high temperature limit setting and shows;


【Export】 : Export counting records and saved as excel file;

【Clean】 : Clear the total records.

3.2.2 Snapshot Folder

To click the **【Snapshot Folder】** , you can check all the captured face pics.

Notice: The folder is named by the date.

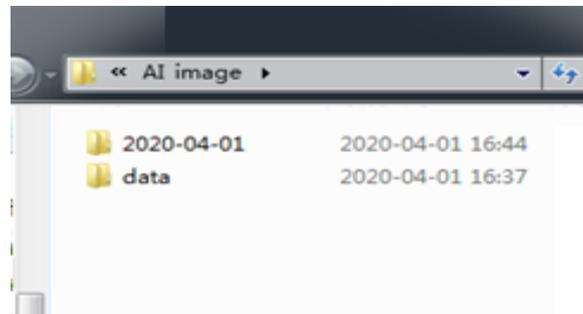

3.2.3Setting

Click **【Setting】** button to enter into the interface to modify the setting;

【Alarm switch】 : Turn On/Off to temperature alarm function;

【High Limit°C】 : Alarm When detecting temperature higher than the high limit°C;

【Duration(S)】 : Temperature alarm duration time, default is 10 seconds;

【Face duplication (0-1)】 : Same people only capture once, no repeat snapshot;

【Capture Interv (MS)】 : The interval time of Same people repeat face capture;



【Correction mode】 : Auto correction or manual adjustment

【Outdoor mode(0-1)】 : 0 indicates aisle environment,1 indicates indoor environment;

【Correction°C】 : Under the severe environment ,it will increase the compensation temperature to improve the accuracy of temperature measurement, time-of-use compensation can be set.

【Lower temperature】 : To set lower temperature

【Detection zone switch】 : On/Off (click “detection zone setting” to set detection area by dragging the drawing line)

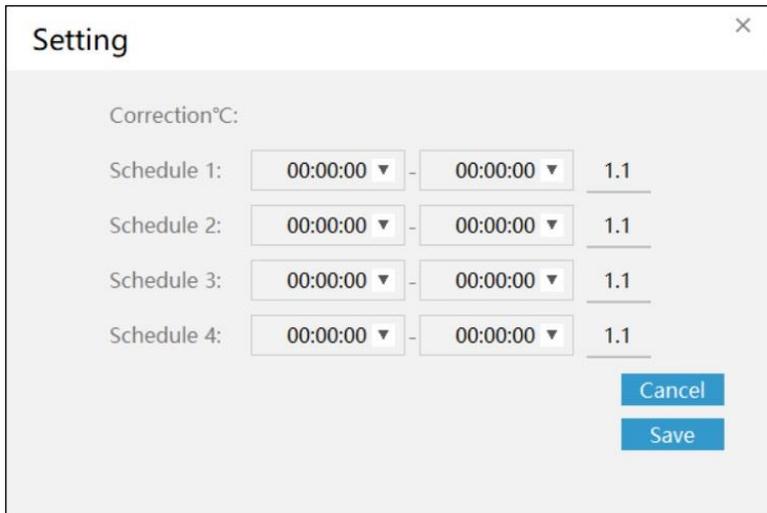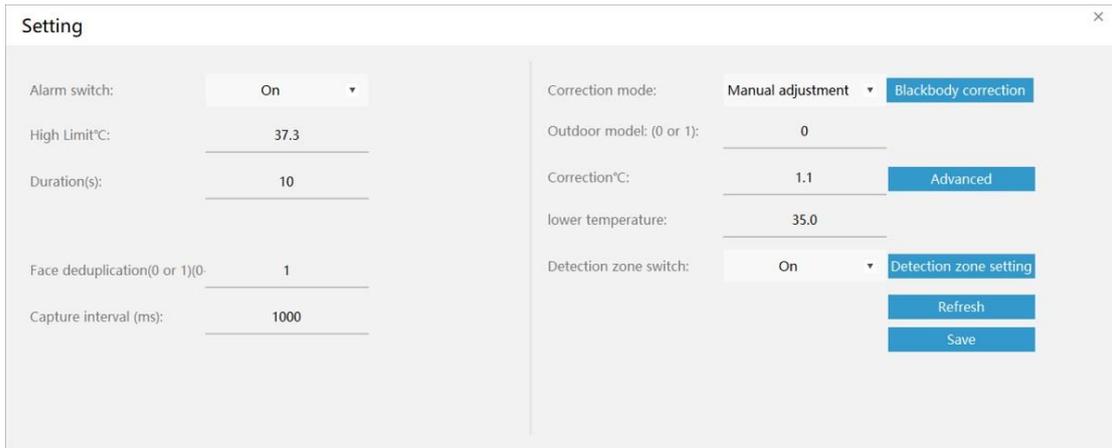

4. Device Upgrade

Users can use browser or PC tool for upgrade;

Notice: Brower upgrade package suffix is .ifu. PC tool upgrade package suffix is .bin

4.1 Web Upgrade

Notice: Only IE browser, QQ browser, and 360 security browser is workable; IE Edge browser, 360 speed browser are not able to use.


Step 1: Open Browser, input device IP address, and input the user name" admin" and password" admin".



Step 2: Click "setting"- "Setting"- "Maintain" to enter into the upgrade interface;


Step 3: Click" Browse" to choose "app.ifu" upgrade file;

Step 4: Click “Upload” button to start upgrading, after upgrade completed, the web page will auto-refresh.

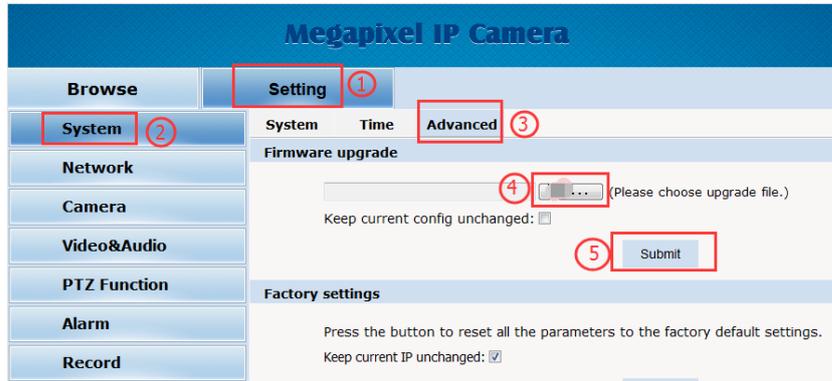

4.2 Tool Upgrade Program:

Step 1: Open the PC to search tool **IPWIZARD** and above version, select the device and upgrade directly for single device;

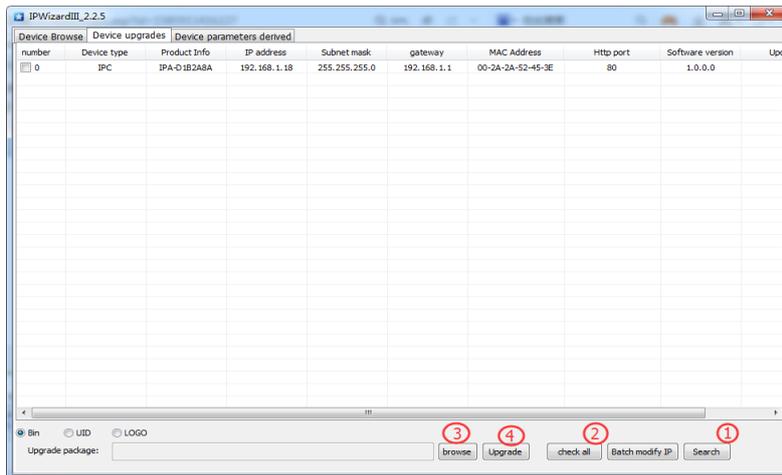

Step 2: For multi-devices batch upgrade, user need to modify the default IP address to different one to avoid IP address collision. Take an example as below pic shows:

